


## DRILL SEQUENCE (CGS4000)


The chart below illustrates the recommended drilling sequence for BioHorizons Tapered implants.<sup>†</sup> Clinical judgement with respect to each individual patient must supersede any recommendation made.

Guided surgery drills include lengths of 17, 21, 24, and 28mm and the standard diameters for BioHorizons Tapered implants.<sup>‡</sup> 17mm drills have depth markings, should they need to be used without the guide.

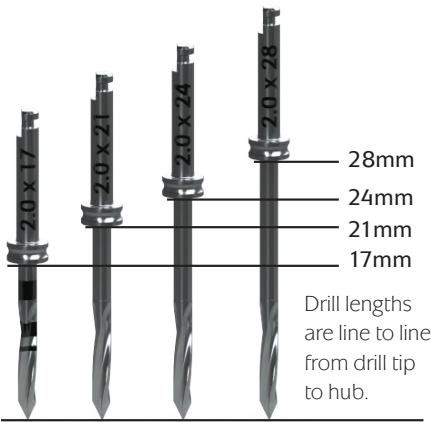

28mm  
24mm  
21mm  
17mm

Drill lengths are line to line from drill tip to hub.

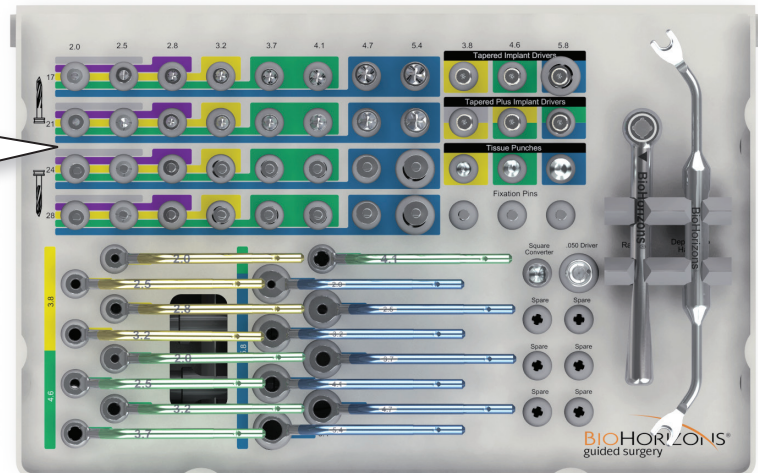

	Pilot Drill	CGS Width Increasing Drills (implant diameter specific)							Implant Driver <sup>†</sup>	
3.0mm body diameter										
3.4mm body diameter										
3.8mm body diameter										
4.2mm body diameter										
4.6mm body diameter										
5.2mm body diameter										
5.8mm body diameter										
		2.0mm pilot	2.5mm width	2.8mm width	3.2mm width	3.7mm width	4.1mm width	4.7mm width <sup>‡</sup>	5.4mm width <sup>‡</sup>	5.8mm width <sup>‡</sup>
	Use to set osteotomy depth	Incrementally widen the osteotomy							Place implant matching the length of the prepared osteotomy	

<sup>†</sup>Mount-free Tapered Internal, Tapered Plus, Tapered 3.0, Tapered Tissue Level. <sup>‡</sup>5.8mm instruments sold separately.



L02029

\*REV B NOV 2019\*  
REV B NOV 2019

customer care: 888.246.8338  
shop online at [store.biohorizons.com](http://store.biohorizons.com)

©BioHorizons. All Rights Reserved. Images shown not to scale.